

# Amplite™ Fluorimetric Acetylcholinesterase Assay Kit

## \*Red Fluorescence\*

Ordering Information:	Storage Conditions:	Instrument Platform:
Product Number: 11402 (200 assays)	Keep in freezer Avoid exposure to light	Fluorescence microplate readers

### Introduction

Acetylcholinesterase (AChE) is one of the most crucial enzymes for nerve response and function. AChE degrades the neurotransmitter acetylcholine (ACh) into choline and acetic acid. It is mainly found at neuromuscular junctions and cholinergic synapses in the central nervous system, where its activity serves to terminate the synaptic transmission. AChE is also found on the red blood cell membranes, where it constitutes the Yt blood group antigen. AChE inhibitors are among the key drugs approved by the FDA for the management of Alzheimer's disease (AD) and myasthenia gravis. This Amplite™ Fluorimetric Acetylcholinesterase Assay Kit provides one of the most sensitive methods for detecting AChE activity or screening AChE inhibitors in red fluorescence window. The kit uses Amplite Red™ to quantify the choline produced from the hydrolysis of acetylcholine by AChE through choline oxidase-mediated enzyme coupling reactions. It can monitor and quantify the AChE activity in blood, cell extracts or other solutions. The fluorescence intensity of Amplite Red™ is used to measure the amount of choline formed, which is proportional to the AChE activity. The kit is an optimized “mix and read” assay that is compatible with HTS liquid handling instruments.

This Amplite™ Fluorimetric Acetylcholinesterase Assay Kit provides a simple one-step fluorometric assay to detect as little as 0.01 mU AChE in a 100 µL assay volume (0.1 mU/mL) as shown in Figure 1. The assay can be performed in a convenient 96-well or 384-well microtiter-plate format and easily adapted to automation without a separation step. Its signal can be easily read with a fluorescence microplate reader at Ex/Em = 540±10/590 ±10 nm (maximum Ex/Em = 540/590 nm) or an absorbance microplate reader at 576±5 nm.

### Kit Key Features

<b>Broad Application:</b>	Can be used for quantifying acetylcholinesterase in solutions and in cell extracts.
<b>Sensitive:</b>	Detect as low as 0.01 mU of acetylcholinesterase in solution.
<b>Continuous:</b>	Easily adapted to automation without a separation step.
<b>Convenient:</b>	Formulated to have minimal hands-on time.

### Kit Components

Components	Amount
Component A: Amplite Red™	1 vial
Component B: Acetylcholinesterase Probe	2 bottles (lyophilized powder)
Component C: Acetylcholinesterase Standard	1 vial (5 units)
Component D: Assay Buffer	1 bottle (25 mL)
Component E: DMSO	1 vial (100 µL)

### Assay Protocol for One 96-well Plate

#### Brief Summary

**Prepare AChE assay mixture (50 µL) → Add AChE standards or AChE test samples (50 µL) → Incubate at room temperature for 10-30 min → Read fluorescence at Ex/Em = 540/590 nm**

*Note: Thaw all the kit components at room temperature before starting the experiment.*




- 4.2 Incubate the reaction at room temperature for 10 to 30 minutes, protected from light.
- 4.3 Monitor the fluorescence increase at Ex/Em = 540/590 nm with a fluorescence microplate reader.

### Data Analysis

The fluorescence in blank wells (with the assay buffer only) is used as a control, and is subtracted from the values for those wells with the acetylcholinesterase reactions. An acetylcholinesterase standard curve is shown in Figure 1.

*Note: The fluorescence background increases with time, thus it is important to subtract the fluorescence intensity value of the blank wells for each data point.*

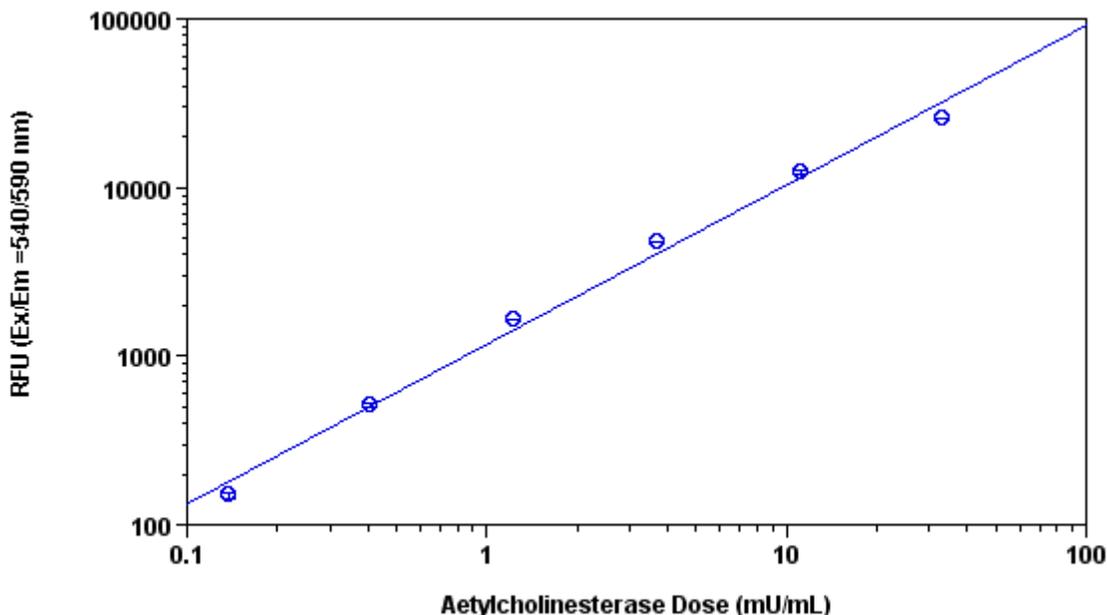

**Figure 1.** Acetylcholinesterase dose response was measured in a 96-well clear plate with Amplite™ Fluorimetric Acetylcholinesterase Assay Kit using a Gemini fluorescence microplate reader (Molecular Devices). As low as 0.01 mU/well (0.1mU/mL) of acetylcholinesterase can be detected with 20 minutes incubation time (n=3).

### References

1. Kovarik, Z et al. (2003). Acetylcholinesterase active centre and gorge conformations analysed by combinatorial mutations and enantiomeric phosphonates. *Biochem. J.* (2003) 373, 33–40.
2. Ordentlich, A. et al. (1996). The Architecture of Human Acetylcholinesterase Active Center Probed by Interactions with Selected Organophosphate Inhibitors. *J. Biol. Chem.* 271 (20):11953–11962.
3. Magnottl, RA. et al. (1987). Measurement of Acetylcholinesterase in Erythrocytes in the Field. *Clin. Chem.* 33/10, 1731-1 735.

**Warning: This kit is only sold to end users. Neither resale nor transfer to a third party is allowed without written permission from AAT Bioquest. Chemical analysis of kit components is strictly prohibited. Please call us at 408-733-1055 or e-mail us at [info@aatbio.com](mailto:info@aatbio.com) if you have any questions.**